



## ISTITUTO NAZIONALE DI RICERCA METROLOGICA Repository Istituzionale

### On the Calibration of Direct-Current Current Transformers (DCCT)

This is the author's submitted version of the contribution published as:

*Original*

On the Calibration of Direct-Current Current Transformers (DCCT) / Callegaro, Luca; Cassiago, Cristina; Gasparotto, E.. - In: IEEE TRANSACTIONS ON INSTRUMENTATION AND MEASUREMENT. - ISSN 0018-9456. - 64:3(2015), pp. 723-727. [10.1109/TIM.2014.2359812]

*Availability:*

This version is available at: 11696/32734 since: 2021-02-19T22:37:13Z

*Publisher:*

IEEE

*Published*

DOI:10.1109/TIM.2014.2359812

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

IEEE

© 20XX IEEE. Personal use of this material is permitted. Permission from IEEE must be obtained for all other uses, in any current or future media, including reprinting/republishing this material for advertising or promotional purposes, creating new collective works, for resale or redistribution to servers or lists, or reuse of any copyrighted component of this work in other works

(Article begins on next page)

# On the calibration of direct-current current transformers

Luca Callegaro, Cristina Cassiago, and Enrico Gasparotto <sup>†</sup>

## Abstract

Modern commercial direct-current current transformers (DCCT) can measure currents up to the kA range with accuracies better than  $1 \times 10^{-5}$ . We discuss here a DCCT calibration method and its implementation with commercial instruments typically employed in low resistance calibration laboratories. The primary current ranges up to 2 kA; in the current range below 100 A the calibration uncertainty is better than  $3 \times 10^{-7}$ . An example of calibration of a high-performance DCCT specified for primary currents measurement up to 900 A is discussed in detail.

## 1. INTRODUCTION

Commercial direct-current current transformers (DCCT) are the most accurate dc high-current sensors available [1], with specified relative accuracies in the  $10^{-5}$  range and integral linearities better than  $1 \times 10^{-6}$ . The verification of such high performances, and the calibration of the DCCT ratio, ask for metrological facilities capable of handling the high currents required, of high accuracy and with automated operability [2–5].

Ultimate current ratio accuracy is achieved in cryogenic current comparators (CCC) [6]. In a CCC, the ratio accuracy is given by constraining the magnetic flux path (generated by the current being compared) within superconducting shields; an extreme sensitivity is given by a superconducting quantum interference device (SQUID) flux sensor. Even though CCCs capable of handling currents up to 100 A have been realized [7], these devices are research instruments not available in calibration laboratories.

Ferromagnetic-core, room-temperature current comparators (CC) are current ratio devices which can achieve ratio errors (deviations from reading) better than  $1 \times 10^{-7}$  [8], and can be self-calibrated through step-up procedures [9, 10] with similar levels of uncertainty. Thus, a CC can act as the current ratio standard in a DCCT calibration setup. Although complex and expensive instruments, high-current CC are a common presence in electrical calibration laboratories, since they are embedded within commercial resistance ratio bridges employed for the measurement of low-valued resistance standards. Such instruments include also current sources, detectors, and firmware for automated operation.

Here we present a simple circuit that allows the calibration of the ratio of a DCCT by using commercial components, originally designed for the calibration of low-valued resistors. The accuracy reached is dependent on the primary current and can be lower than  $3 \times 10^{-7}$  for currents below 100 A. An example of calibration of a DCCT having a 1500 : 1 nominal ratio for currents up to 900 A is reported.

The implementation has been employed for the participation to the EURAMET.EM-S35 High DC current ratio supplementary comparison [11], in which INRIM acts as co-pilot laboratory.

## 2. THE METHOD

Fig. 1 shows the schematics of the calibration setup.

The instruments employed are, in addition to the DCCT under calibration, an automated current range extender EXT and a current comparator ratio bridge CC.

All these instruments are based on the same principle: a high-permeability ferromagnetic core is wound by  $m + 1$  windings, each of  $N_k$  turns, through which currents  $I_k$  flow. The magnetic equation of such circuit is  $\sum_k N_k I_k = \mathcal{R} \Phi$ , where  $\Phi$  is the flux in the magnetic core and  $\mathcal{R}$  its magnetic reluctance.  $\Phi$  is measured by a dc flux detector (based on the fluxgate modulation technique [1, 12, 13]) which output acts as error signal for the feedback control of a current generator  $I_0$  connected to winding  $N_0$ . The goal of the feedback control is to achieve  $\Phi = 0$ , which results in the ampere-turns balance equation  $\sum_{k=0}^m N_k I_k = 0$ .

In both DCCT and EXT, only two windings ( $m = 1$ ) are active in a given operating condition. The controlled current generator output  $I_0$  constitutes the device output current; the primary current  $I_1$  is

<sup>\*</sup>Luca Callegaro, Cristina Cassiago and Enrico Gasparotto are with the Electromagnetism Division of the Istituto Nazionale di Ricerca Metrologica (INRIM), Strada delle Cacce 91, 10135 Torino, Italy, e-mail: l.callegaro@inrim.it

<sup>†</sup>Manuscript received March 4, 2014.

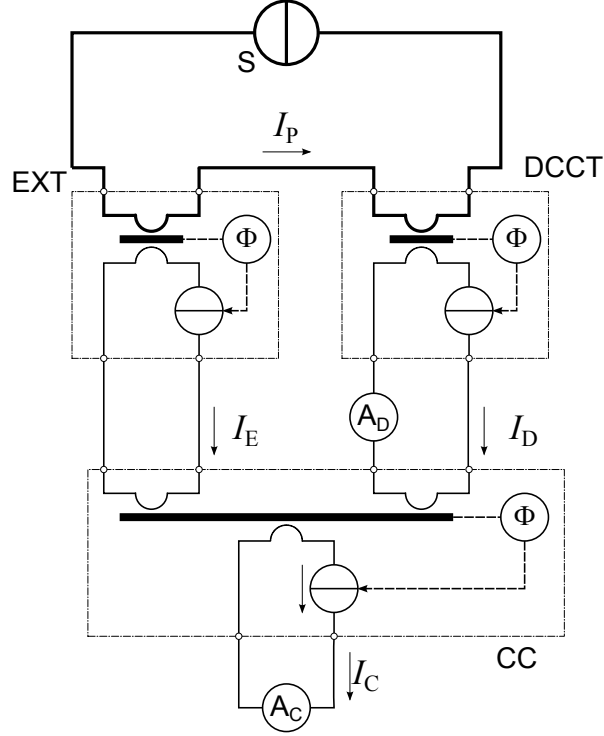


Figure 1: Principle schematics of the DCCT calibration setup.  $S$  is the high-current source,  $EXT$  is an automated current range extender,  $CC$  a dc current comparator. Meter  $A_D$  monitors the DCCT output  $I_D$ ; meter  $A_C$  give the reading of  $I_C$  employed in the measurement model Eq. (2).

thus scaled down with the turns ratio  $t = \frac{N_1}{N_0}$  as  $I_0 = tI_1$ . In CC, more windings ( $m \geq 2$ ) are active; currents can be compared, weighted by their respective winding turns; a measurement of the controlled current generator output allows the determination of the primary current unbalances.

In Fig. 1, the input windings of both DCCT and EXT, are connected in series and fed by the primary current  $I_P$  generated by a high-current dc source  $S$ . DCCT and EXT output currents are  $I_D = G_D I_P$ , and  $I_E = G_E I_P$  respectively;  $G_D$  is the DCCT current gain (that is, the measurand), and  $G_E$  is the EXT current gain.

$I_D$  and  $I_E$  are connected to two input windings of CC, each having  $N_D$  and  $N_E$  turns.  $I_D$  is also measured by a high-accuracy ammeter  $A_D$ .

The CC compensation current  $I_C$ , linked to CC winding of turns  $N_C$ , is measured by ammeter  $A_C$ ; when operating properly, the CC balance equation is

$$N_E I_E + N_D I_D + N_C I_C = 0. \quad (1)$$

In Eq. (1), the sign of turn numbers  $N_x$  can be either positive or negative and is set by the winding direction on the core.

When all automated controls operate properly, each core flux is drawn to zero, and the balance equation is of the whole circuit becomes

$$G_D = \frac{I_C}{I_P} \frac{N_C}{N_D} - G_E \frac{N_E}{N_D}. \quad (2)$$

A relative gain error  $\delta G_D$  respect to nominal gain  $G_D^{(n)}$  can also be computed,

$$\delta G_D = \frac{G_D - G_D^{(n)}}{G_D^{(n)}}. \quad (3)$$

All instruments based on the fluxgate technique suffer from a certain degree of dc offset, caused by the magnetization hysteresis and relaxation of the ferromagnetic core. This offset, in the order of  $1 \times 10^{-5}$  A per unit input turn [12], is dependent on temperature, measurement history and drifts with time. To compensate for these offset, the reading  $I_C$  in Eq. (2) is substituted with  $\Delta I_C = I_C - I_{C0}$ , where  $I_{C0}$  is the reading taken with null primary current  $I_P = 0$ .

### 3. IMPLEMENTATION

A test implementation of the schematic of Fig. 1 has been set up with the following instrumentation:

- DCCT under calibration. Results reported in Sec. 4. refer to a LEM mod. ITN 900-S ULTRASTAB high-performance current transducer [14]. Primary current  $|I_P| \leq 900$  A, nominal ratio  $G_D = 1/1500$ , accuracy better than  $2 \times 10^{-5}$  (including offset), linearity better than  $1 \times 10^{-6}$ , maximum resistance of the burden  $2.5 \Omega$ . Fig. 2 shows the DCCT mounted on the primary busbar.

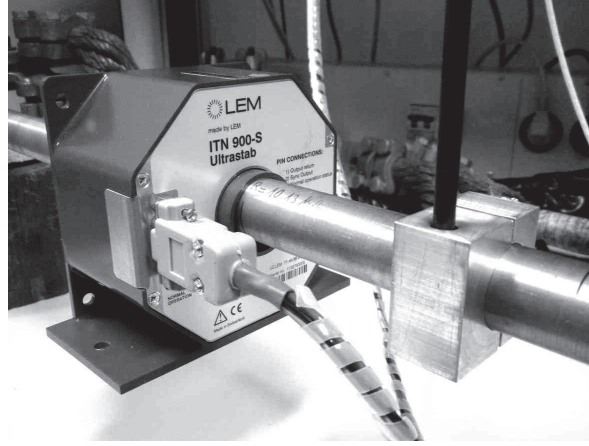


Figure 2: The DCCT under calibration mounted on the primary current busbar. Placed on the busbar is also an aluminum block (foreground) that includes a thermometer head for temperature monitoring.

- CC: Guildline mod. 9920 direct current comparator. This instrument is particularly flexible since it provides several fixed windings having a decadic (1 to 1000) number of turns, one winding with an adjustable number of turns through decade rotary switches, and allows a full reconfiguration of the connections between the windings and the internal electronics. The setting for the DCCT being calibrated is  $N_D = -100$  (fixed winding),  $N_E = 150$  (decade winding).  $N_C = 1$ , in order to achieve the largest sensitivity in the measurement of  $I_C$ .
- EXT: Two different extenders have been employed, depending on  $I_P$ :
  - Measurement International mod. MI 6011B range extender.  $|I_P| \leq 100$  A, nominal ratio  $1/1000$ , relative accuracy  $< 1 \times 10^{-7}$ .
  - Measurement International mod. MI 6012M range extender,  $|I_P| \leq 2$  kA, nominal ratio  $1/1000$ , relative accuracy  $< 2 \times 10^{-6}$ .

The performances of these instruments can be validated in the original low-resistance measurement setups for which they are designed [15].

- S: two different sources have been employed, depending on the primary current  $I_P$ :

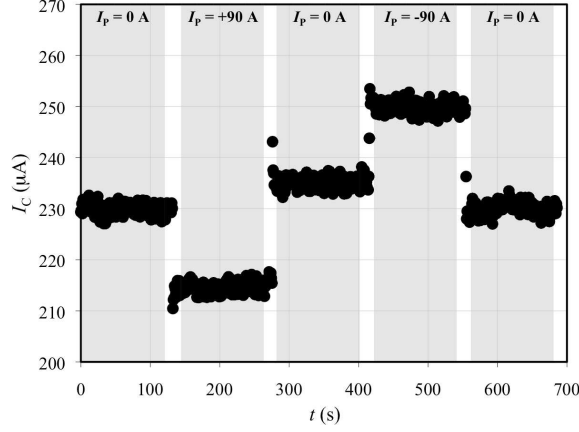


Figure 3: Time recording of the compensation current  $I_C$  for different primary currents  $I_P$ .

- Measurement International MI 6100A linear dc power supply, current output 0 A to +100 A. Current reversal is achieved with a switch internal to MI 6011B.
- Agilent mod. 6680A, current output up to 875 A. Two items are connected in parallel, and a Measurement International mod. 6025 pneumatic switch allows the current reversal.
- $A_D$ : an Agilent mod. 3458A multimeter, in dc voltage mode, measures the voltage drop on a Tinsley mod. 1659  $1\ \Omega$  standard resistor.
- $A_C$ : a second 3458A multimeter in dc current mode, 100 mA range.

The DCCT and busbar temperatures are monitored with two PT100 platinum thermoresistance elements read by a Fluke mod. 1529 CHUB E-4 thermometer. Fig. 2 shows the location of the busbar thermometer head.

#### 4. RESULTS

The gain error  $\delta G_D$  defined in Sec. 2. asks for the determination of  $\Delta I_C = I_C - I_{C0}$ , where the two readings  $I_C$  and  $I_{C0}$  correspond to the nominal current  $I_P^{(n)}$  of interest, and to a zero current  $I_P = 0$ . The measurement system is therefore run continuously, and  $I_P$  is cycled periodically between values 0,  $+I_P^{(n)}$ , 0,  $-I_P^{(n)}$  and so on; the reading  $I_C$  is continuously recorded. Fig. 3 shows a time series of  $I_C$  readings corresponding to an  $I_P$  cycle. For each value of  $I_P$ , after transients have died out, a time average  $\overline{I_C}(I_P)$  is computed (see gray bands in Fig. 3).

The quantity  $\Delta I_C$  to be employed in Eq. (2) is computed as  $\Delta I_C(I_P^{(n)}) = \overline{I_C}(I_P^{(n)}) - (\overline{I_C}'(0) + \overline{I_C}''(0))/2$ , where  $\overline{I_C}'(0)$  and  $\overline{I_C}''(0)$  are the zero readings respectively preceding and succeeding  $\overline{I_C}(I_P^{(n)})$  in the time series.

From each  $\Delta I_C(I_P^{(n)})$ , the absolute  $\Delta G_C(I_P^{(n)})$  and relative  $\delta G_C(I_P^{(n)})$  errors are computed. Fig. 4 graphically shows the values  $\delta G_D$  corresponding to each  $I_P^{(n)}$  measurement cycle. Tab. 1 reports the estimates for  $G_D$  and  $\delta G_D$  of the DCCT under measurement, together with the corresponding 95 % expanded uncertainties, for several primary current  $I_P^{(n)}$  values.

As an example, the uncertainty budget for the calibration of  $G_D$  at  $I_P = +90$  A is given in Tab. 2, where it can be appreciated that the principal contributions to measurement uncertainty are the measurement repeatability of  $I_C$  and the EXT ratio  $N_E/N_D$ .

#### 5. CONCLUSIONS

The setup proposed allows the calibration of the ratio of a DCCT with accuracies in the  $10^{-6}$  range or better. The proposed implementation, suitable for primary currents up to 2 kA, is based on commercial

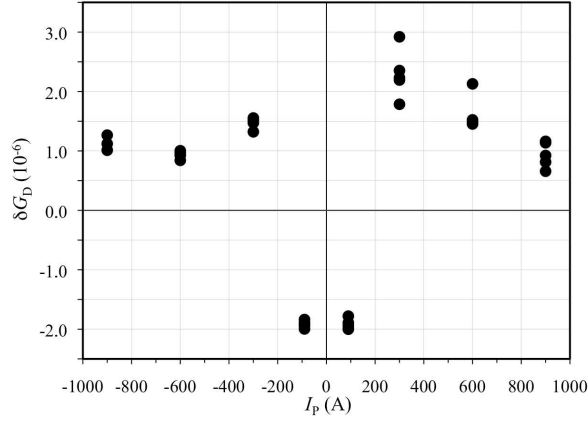


Figure 4: The relative gain error  $\delta G_D$  of the DCCT under calibration, for different nominal primary current values  $I_p^{(n)}$ . Each dot corresponds to half of the measurement cycle shown in Fig. 3. For each  $I_p^{(n)}$ , five measurement results are reported. The average value and its uncertainty are given in Tab. 1.

Table 1: DCCT gain  $G_D$  for different primary currents  $I_p$ . The relative deviation  $\delta G_D$  from nominal ratio is also reported.

$I_p^{(n)}$ A	Supply	EXT	$G_D$ $\times 10^{-4}$	$\delta G_D$ $\times 10^{-6}$	$U(\delta G_D)$ $\times 10^{-6}$
+90	6100A	6011B	6.666 653 9(16)	-1.92	0.24
-90	6100A	6011B	6.666 653 9(16)	-1.92	0.23
+300	6680A	6012M	6.666 682(16)	+2.3	2.3
-300	6680A	6012M	6.666 676(15)	+1.5	2.3
+600	6680A	6012M	6.666 677(15)	+1.6	2.3
-600	6680A	6012M	6.666 676(15)	+0.9	2.3
+900	6680A	6012M	6.666 672(15)	+0.9	2.3
-900	6680A	6012M	6.666 673(15)	+1.1	2.3

instruments typically employed for low-resistance calibrations, and therefore often available in calibration laboratories. The implementation has been employed for the participation to the EURAMET.EM-S35 comparison. The result of the comparison, when available, will therefore constitute a validation of the implementation.

#### ACKNOWLEDGMENTS

The authors are indebted with Alessandro Mortara, Bundesamt für Metrologie (METAS), Switzerland, for fruitful discussions; and with their colleague Fulvio Francone for help in the construction of the calibration facility.

#### REFERENCES

- [1] P. Ripka, “Electric current sensors: a review,” *Meas. Sci. Technol.*, vol. 21, p. 112001, 2010, 23 pp.
- [2] M. Zhu and K. Xu, “A calibrating device for large direct current instruments up to 320 kiloampere-turns,” *Instrumentation and Measurement, IEEE Transactions on*, vol. 47, no. 3, pp. 711–714, Jun 1998.
- [3] G. Fernqvist, J. Pett, and J. Pickering, “A reference standard system based on dc current,” in *Precision Electromagnetic Measurements, 2002. Conference Digest 2002 Conference on*, June 2002, pp. 164–165.
- [4] G. Fernqvist, B. Halvarsson, J. Pett, and J. Pickering, “A novel current calibration system up to 20 kA,” *Instrumentation and Measurement, IEEE Transactions on*, vol. 52, no. 2, pp. 445–448, April 2003.

Table 2: Uncertainty budget for  $G_D$ , at  $I_p^{(n)} = +90$  A.

Quantity	$X$	$u(X)$	contrib. to $u(G_D)$	type
$\Delta I_C$	$-17.2 \mu\text{A}$	$0.36 \mu\text{A}$	$2.7 \times 10^{-11}$	A
$I_P$	90 A	90 mA	$1.3 \times 10^{-12}$	B
$N_C/N_D$	$-6.666\,666\,7 \times 10^{-3}$	$6.7 \times 10^{-10}$	$< 1 \times 10^{-13}$	B
$N_E/N_D$	$-6.666\,666\,7 \times 10^{-1}$	$6.7 \times 10^{-8}$	$6.7 \times 10^{-11}$	B
$G_E$	$+1.000\,000\,0 \times 10^{-3}$	$5.8 \times 10^{-11}$	$3.8 \times 10^{-11}$	B
$G_D$	$+6.666\,653\,9 \times 10^{-4}$	$8.1 \times 10^{-11}$		
$\delta G_D$	$-1.92 \times 10^{-6}$	$1.2 \times 10^{-7}$		
$U_{R95}(\delta G_D)$		$2.4 \times 10^{-7}$		

- [5] G. Hudson, B. Jeckelmann, and J.-D. Baumgartner, “Comparison of cern and metas high current standards up to 10ka,” in *Precision Electromagnetic Measurements Digest, 2008. CPEM 2008. Conference on*, June 2008, pp. 548–549.
- [6] J. M. Williams, “Cryogenic current comparators and their application to electrical metrology,” *IET Science, Measurement & Technology*, vol. 5, no. 6, pp. 211–224, 2011.
- [7] J. M. Williams and P. Kleinschmidt, “A cryogenic current comparator bridge for resistance measurements at currents of up to 100 A,” *IEEE Trans. Instr. Meas.*, vol. 48, no. 2, pp. 375–378, 1999.
- [8] W. J. M. Moore and P. N. Miljanic, *The current comparator*, ser. IEE electrical measurement series. London, UK: Peter Peregrinus Ltd, 1988, vol. 4, iSBN 0863411126.
- [9] H. Shao, F. Lin, X. Hua, B. Liang, K. Qu, and Y. Pan, “DC high current ratio standard based on series-parallel calibration method,” in *Precision Electromagnetic Measurements (CPEM) Conf.*, Jun. 2010, pp. 535–536.
- [10] H.-G. Zhao, X.-Z. Zhang, Y. Liu, L.-Y. Zheng, and B.-X. Zou, “Calibration of DC current up to 600 A,” in *Precision Electromagnetic Measurements (CPEM) Conf. on*, Jun. 2010, pp. 603–604.
- [11] C. Cassiago and A. Mortara, “Comparison of high-current ratio standard,” EURAMET, Technical Protocol 1217, Feb 2012, available online at [www.euramet.org](http://www.euramet.org).
- [12] M. P. MacMartin and N. L. Kusters, “A direct-current-comparator ratio bridge for four-terminal resistance measurements,” *IEEE Trans. Instr. Meas.*, vol. 15, no. 4, pp. 212–220, Dec 1966.
- [13] P. Odier, “DCCT technology review,” in *Proc. of Workshop on DC current transformers and beam-lifetime evaluations*, A. Peters, H. Schmickler, and K. Wittenburg, Eds. Lyon, France: CARE-HHH-ABI Networking, 1-2 Dec 2004, pp. 3–5.
- [14] W. Teppan and D. Azzoni, “Closed-loop fluxgate current sensor,” European Patent EP2 251 704A1, 2010.
- [15] M. Kraft, “Measurement techniques for evaluating current range extenders from 1 ampere to 3000 ampere,” *NCSLI Measure J. Meas. Sci.*, vol. 7, no. 3, pp. 32–36, Sep 2012.