



ISTITUTO NAZIONALE DI RICERCA METROLOGICA Repository Istituzionale

Metrological traceability paths for stable isotope measurements of CO₂ in air

Original

Metrological traceability paths for stable isotope measurements of CO₂ in air / Sega, Michela; Rolle, Francesca; Durbiano, Francesca; Pavarelli, Stefano; Pennechi, Francesca Romana; Russo, Ramona; Festevole, Chiara. - (2025), pp. 7-10. (Joint IMEKO TC8, TC11, TC24 Conference 2025 Torino (Italy) 14-17 September 2025).

Availability:

This version is available at: 11696/88467 since: 2026-02-27T15:41:08Z

Publisher:

Published

DOI:

Terms of use:

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

Publisher copyright

IMEKO
© IMEKO

(Article begins on next page)

Metrological traceability paths for stable isotope measurements of CO₂ in air

Michela Segal^{1*}, Francesca Rolle¹, Francesca Durbiano¹, Stefano Pavarelli¹, Francesca Romana Pennechi¹, Ramona Russo^{1,2}, Chiara Festevole³

¹ INRiM Istituto Nazionale di Ricerca Metrologica, Strada delle Cacce 91
10135 Torino (IT), m.sega@inrim.it, f.rolle@inrim.it, f.durbiano@inrim.it, s.pavarelli@inrim.it,
f.pennechi@inrim.it, r.russo@inrim.it

² DENERG Dipartimento Energia, Politecnico di Torino, Corso Duca degli Abruzzi 24
10129 Torino (IT), ramona.russo@polito.it

³ Dipartimento di Chimica, Università degli Studi di Torino, Via P. Giuria 7,
10125 Torino (IT), chiara.festevole@edu.unito.it

Abstract – Measurements of carbon stable isotopes ¹³C and ¹²C and of their ratio ¹³C/¹²C in atmospheric carbon dioxide ($\delta^{13}\text{C-CO}_2$) are indicators of the anthropogenic contribution to CO₂ emissions. At present, $\delta^{13}\text{C-CO}_2$ falls within the CIPM MRA traceability exception. Gaseous Certified Reference Materials (CRMs) are needed as proper references to support the scientific community dealing with $\delta^{13}\text{C-CO}_2$ in atmospheric measurements. The paper presents an approach to assign $\delta^{13}\text{C-CO}_2$ values to CO₂ gas mixtures at atmospheric amount fraction following two independent traceability paths, leading to candidate CRMs with established metrological traceability to the Vienna Pee Dee Belemnite scale, which represents an international recognized primary scale in this framework. INRiM is working towards the attainment of internationally recognized Calibration and Measurement Capabilities in the CIPM MRA framework for the production of such CRMs, which represents a fundamental step to meet the increasing demand of proper references for stable carbon isotopes measurements in atmosphere.

I. INTRODUCTION

Measurements of carbon stable isotopes ¹³C and ¹²C and of their ratio ¹³C/¹²C ($\delta^{13}\text{C}$) in atmospheric carbon dioxide ($\delta^{13}\text{C-CO}_2$), are indicators of the anthropogenic contribution to CO₂ emissions. These measurements provide useful data to monitor the anthropogenic CO₂ impact on climate change. Indeed, the carbon isotopic composition of atmospheric CO₂ has substantially changed compared to the pre-industrial era mainly due to human activities which influence the natural carbon cycle [1]. As a result, while the atmospheric CO₂ concentration is continuously raising [2], the value of $\delta^{13}\text{C-CO}_2$ decreases [3]. In order to ensure the reliability of CO₂ amount fraction and $\delta^{13}\text{C-CO}_2$ measurement results, they have to

be traceable to internationally recognized references, which enable data comparability in time and space. However, delta value isotope ratio measurements that cannot be traceable to SI fall in a traceability exception of the CIPM Mutual Recognition Arrangement (CIPM MRA) and should be made traceable to materials recognised as International Standards [4]. Since at present, values assigned to these materials are based on consensus values, these materials are not listed in the Appendix C of the BIPM Database [5]. Concerning $\delta^{13}\text{C}$ in CO₂, its metrological traceability relies on an unbroken chain of calibrations linking the measurement results to the international primary carbon isotope delta scale, namely the Vienna Pee Dee Belemnite (VPDB) [6]. The International Atomic Energy Agency (IAEA) is recognized as the custodian of stable isotope ratio measurement scales for light elements, including carbon. The VPDB isotope reference defines the zero point of the carbon stable isotope scale describing the relative abundance of ¹³C and ¹²C. At present, the standard and associated VPDB scale for $\delta^{13}\text{C}_{\text{VPDB}}$ in CO₂ are artefact-based and rely on the CO₂ production from carbonate material through its reaction with (over)saturated phosphoric acid. They are used to transfer the scale to CO₂ in air measurements. The Max Planck Institute for Biogeochemistry (MPI-BGC), in its capacity as World Metrological Organization (WMO) Central Calibration Laboratory, developed the Jena reference air set (JRAS) which is anchored to the VPDB scale [7]. However, the use of this method is limited to specialized laboratories and gaseous Certified Reference Materials (CRMs) are needed to meet increasing demand. Recently, another carbon isotope delta scale, the VPDB-LSVEC (LSVEC – lithium carbonate prepared by H. J. Svec), was accepted as another international primary scale by the scientific community expert on the subject of stable isotopes [6]. VPDB-LSVEC is also an artefact-based scale and, as carbon isotope delta values reported on the VPDB and VPDB-LSVEC scales can differ, conversion models

between the two scales can be established and used but they will introduce additional uncertainty contribution. At INRiM, following the participation in the European Joint Research Projects EMPIR 16ENV06 SIRS [8] and EMPIR 19ENV05 STELLAR [9], and in compliance with the prescriptions of the relevant ISO standard [10], gravimetric mixtures of CO₂ at atmospheric amount fraction in air, considered as candidate CRMs for isotopic composition, are under development [11,12]. They are based on two different traceability paths, both linked to the VPDB scale. The first path relies on pure CO₂ sources having different $\delta^{13}\text{C-CO}_2$ values considered as references, which are diluted to ambient amount fraction to produce the candidate CRMs. The second one starts from certified reference mixtures, which are employed to calibrate a cavity ring-down spectrometer (CRDS) used to assign the isotopic values to the same candidate CRMs. This work presents the two traceability paths and their application to three case studies at different $\delta^{13}\text{C-CO}_2$ values.

II. MATERIALS AND METHODS

In the presented approach, the production of CO₂ mixtures at ambient amount fraction in synthetic air (SA) with known $\delta^{13}\text{C-CO}_2$ value started from two pure gas sources of CO₂, one having a depleted value and the other having an enriched value of $\delta^{13}\text{C-CO}_2$ (SIAD, Italy). Aliquots of the pure CO₂ sources were sampled in 1 L-gas flasks and sent to MPI-BGC for the value assignment by IRMS on the VPDB scale. Blending the two pure CO₂ sources allowed to obtain also a third intermediate $\delta^{13}\text{C-CO}_2$ value.

The pure CO₂ sources were diluted in subsequent steps by applying the gravimetric method [13]. The dilution was carried out using pure gases, i.e. nitrogen (N₂) 6.0 (Air Liquide Italia, Italy), argon (Ar) 7.0 (Linde, Germany), and oxygen (O₂) 6.0 (Air Liquide Italia, Italy), to obtain 3 mixtures of CO₂ at ambient amount fraction in SA, INRiM A, INRiM B, and INRiM C, at different $\delta^{13}\text{C-CO}_2$ values. The mixtures were prepared in 5 L high-pressure cylinders of aluminium alloy (Luxfer, UK).

The gravimetrically prepared mixtures underwent an analytical verification by CRDS (CRDS G2131-i, Picarro, USA). This step allowed to determine an analytical $\delta^{13}\text{C-CO}_2$ value linked to VPDB by an independent traceability path. The CRDS was indeed calibrated by means of CO₂ gas standards in SA previously prepared by gravimetry from different pure CO₂ sources, having $\delta^{13}\text{C-CO}_2$ values assigned via IRMS at MPI-BGC on the JRAS-06 scale.

The entire process is depicted in Figure 1. Details on the various steps are reported in the sub-sections below.

Table 1 summarises the characteristics of the candidate CRMs to be produced following the described procedure.

Table 1. Characteristics of the candidate CRMs of CO₂ in SA at atmospheric amount fraction with known $\delta^{13}\text{C-CO}_2$ values.

Mixture code	Nominal CO ₂ amount fraction, $\mu\text{mol/mol}$	Nominal $\delta^{13}\text{C-CO}_2$ value, ‰
INRiM A	410	+1.2
INRiM B	410	-42
INRiM C	410	-21

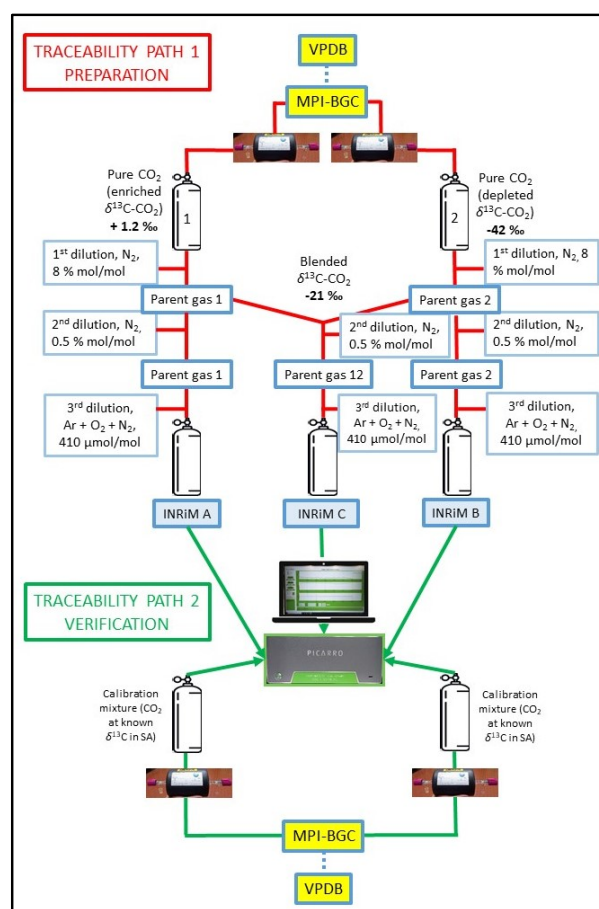


Fig. 1. Schematic of the production process of candidate CRMs of CO₂ in SA at atmospheric amount fraction with known $\delta^{13}\text{C-CO}_2$ values.

III. METROLOGICAL TRACEABILITY PATH 1 – GRAVIMETRIC PREPARATION

The gravimetric preparation of CO₂ mixtures in SA at ambient amount fractions starting from pure gases cannot be carried out in a single step, as illustrated in Figure 1. This is due to the fact that the mass of gases to be

introduced into the cylinders must be high enough to guarantee a good performance of the weighing system. The gravimetric dilution has the great advantage that it allows to obtain final mixtures with the same $\delta^{13}\text{C-CO}_2$ value of the pure source CO_2 .

Each of the two pure gas sources of CO_2 was diluted in N_2 6.0 to prepare a first parent mixture having CO_2 nominal amount fraction of 8 % mol/mol; a second parent mixture was then prepared to reach a CO_2 nominal amount fraction of 0.5 % mol/mol.

The mixtures having nominal CO_2 amount fraction of 410 $\mu\text{mol/mol}$ in SA were then prepared by adding proper masses of Ar 7.0, O_2 6.0 and N_2 6.0. Two mixtures, namely INRiM A at about +1.2 ‰ and INRiM B at about -42 ‰, were obtained. A third mixture, INRiM C, was prepared by blending the two CO_2 sources, targeting an intermediate $\delta^{13}\text{C-CO}_2$ value of about -21 ‰. To optimise the performance of INRiM gravimetric facility and of its mass comparator, the dilution process did not start from the two pure CO_2 , but aliquots of the two parent mixtures of CO_2 in N_2 at 8 % mol/mol were mixed gravimetrically. Two subsequent dilutions were needed to obtain the final INRiM C mixture of CO_2 at atmospheric amount fraction.

IV. METROLOGICAL TRACEABILITY PATH 2 – ANALYTICAL VERIFICATION

The gravimetrically prepared mixtures were verified by CRDS. This analyser allowed the direct measurement of $\delta^{13}\text{C-CO}_2$, and was calibrated with two gas standards bracketing the $\delta^{13}\text{C-CO}_2$ values of the prepared gas mixtures.

To calibrate the CRDS, its analysis curve was determined by fitting the straight-line model (1) by applying the Weighted Total Least Squares implemented by the INRiM Calibration Curves Computing (CCC) software [14]:

$$y = a + bx \quad (1)$$

where:

y is the calculated value of $\delta^{13}\text{C-CO}_2$ in ‰ in the mixture under verification;

a is the intercept of the analysis curve;

b is the slope of the analysis curve;

x is the average of repeated readings ($n = 100$) of the CRDS analyser.

The analysis curve was then used to assign an analytical $\delta^{13}\text{C-CO}_2$ value to each gravimetrically prepared mixture.

V. COMPARISON BETWEEN THE TWO PATHS

The procedure described above allows to assign $\delta^{13}\text{C-CO}_2$ values to gravimetric prepared mixtures of CO_2 in SA by means of two independent techniques having different traceability chains. Usually, path 2 gives a measurement uncertainty associated with the $\delta^{13}\text{C-CO}_2$ value higher than the gravimetric one, as the analytical steps add additional uncertainty sources. However, the possibility of having

two independent values is a strong advantage as the analytical result allows also to verify the goodness of the gravimetric preparation. For this purpose, the two values are compared by calculating the normalized error, E_n , defined in Eq. 2:

$$E_n = \frac{y_{\text{grav}} - y_{\text{CRDS}}}{2 \sqrt{u_{\text{grav}}^2 + u_{\text{CRDS}}^2}} \quad (2)$$

where:

y_{grav} is the $\delta^{13}\text{C-CO}_2$ in ‰ obtained by gravimetry;

y_{CRDS} is the $\delta^{13}\text{C-CO}_2$ in ‰ obtained by CRDS analysis;

u_{grav} is the standard uncertainty associated with y_{grav} ;

u_{CRDS} is the standard uncertainty associated with y_{CRDS} .

If the criterion of Eq. 3 is met

$$-1 \leq E_n \leq 1 \quad (3)$$

the gravimetric value is confirmed, the entire process is demonstrated to be under control and the candidate CRM can be considered valid.

The analytical procedure associated with path 2 can also be used as standalone to directly assign the $\delta^{13}\text{C-CO}_2$ value by CRDS to CO_2 mixtures prepared by means of a less accurate process with respect to gravimetry or produced by external laboratories. The resulting mixture will not be a CRM, but a calibrated gas mixture, accompanied by a calibration certificate.

VI. CONCLUSIONS

At present, $\delta^{13}\text{C}_{\text{VPDB}}$ measurements represent a traceability exception of the CIPM MRA. Gaseous CRMs are needed as proper and more easily accessible references to support the scientific community dealing with CO_2 stable isotopes in air and $\delta^{13}\text{C-CO}_2$ in atmospheric CO_2 measurements. The paper presents an approach to assign $\delta^{13}\text{C-CO}_2$ values to gas mixtures of CO_2 in SA at atmospheric amount fraction following two independent traceability paths, thus leading to candidate CRMs with established metrological traceability to VPDB scale. INRiM is working towards the attainment of internationally recognized Calibration and Measurement Capabilities (CMCs) in the CIPM MRA framework for the production of such CRMs. This represents a fundamental step to meet the increasing demand for proper references for stable carbon isotopes in atmosphere.

Acknowledgements

Part of this work has been funded by the Italian Ministry of University and Research (MUR) in the framework of the project “METRO-INN – National Infrastructure for the quality of measurements for sustainable innovation”, under the Fund for the enhancing of public investments and national development (Law n. 160/2019).

REFERENCES

- [1] H.Graven, R.F.Keeling, J.Rogelj “Changes to Carbon Isotopes in Atmospheric CO₂ Over the Industrial Era and Into the Future”, *Global Biogeochemical Cycles*, 34, e2019GB006170.
- [2] <https://gml.noaa.gov/ccgg/trends/>. Accessed: Apr. 30, 2025.
- [3] https://scrippsco2.ucsd.edu/graphics_gallery/isotopic_data/mauna_loa_and_south_pole_isotopic_c13_ratio.htmlhttps://scrippsco2.ucsd.edu/graphics_gallery/isotopic_data/mauna_loa_and_south_pole_isotopic_c13_ratio.html. Accessed: Apr. 30, 2025.
- [4] “Decision CIPM/104–26, Traceability Exception: Delta Value Isotope Ratio Measurements,” CIPM (2015), <https://www.bipm.org/documents/20126/48101963/Traceability-Exception-QM1>. Accessed: Apr. 28, 2025.
- [5] <https://www.bipm.org/kcdb/>. Accessed: Apr. 30, 2025.
- [6] F.Camin, D.Besic, P.J.Brewer, C.E.Allison, T.B.Coplen, P.J.H.Dunn, M.Gehre, M.Gröning, H.A.J. Meijer, J.-F. Hélie, P.Iacumin, R.Kraft, B.Krajnc, S.Kümmel, S.Lee, J.Meija, Z.Mester, J.Mohn, H.Moossen, H.Qi, G.Skrzypek, P.Sperlich, J.Viallon, L.I.Wassenaar, R.I.Wielgosz “Stable Isotope Reference Materials and Scale Definitions—Outcomes of the 2024 IAEA Experts Meeting”, *Rapid Communications in Mass Spectrometry*, vol.39, No.14, 2025.
- [7] M.Wendeberg, J.M.Richter, M.Rothe, W.A.Brand, “Jena reference air set (JRAS): a multi-point scale anchor for isotope measurements of CO₂ in air”, *Atmos Meas Tech.* vol.6, No.3, 2013, pp.817–822.
- [8] <https://projectsites.vtt.fi/sites/SIRS/>. Accessed: Apr. 28, 2025.
- [9] <http://empir.npl.co.uk/stellarproject/>. Accessed: Apr. 28, 2025.
- [10] ISO, “General Requirements for the Competence of Reference Material Producers (ISO 17034:2016),” International Organization for Standardization, Geneva (Switzerland), 2016.
- [11] F.Rolle, F.Durbiano, S.Pavarelli, F.R.Pennecchi, M.Sega, “Pilot study CCQM-P239 “CO₂ Isotope Ratios (expressed as δ¹³C and δ¹⁸O) in Carbon Dioxide in air mixtures” - INRiM Report, 31, 2024, pp.1-15.
- [12] M.Sega, F.Durbiano, S.Pavarelli, F.R.Pennecchi, F.Rolle, “Comparison of cavity ring-down spectroscopy and Fourier transform infrared spectroscopy for the isotopic composition determination of CRMs of CO₂ in air,” *Proc. of 22nd International Metrology Congress, EPJ Web of Conferences*, 2025, vol.323, pp. 09002, <https://doi.org/10.1051/epjconf/202532309002>.
- [13] ISO 6142: International Standard ISO 6142-1, Gas analysis - Preparation of calibration gas mixtures - Part 1: Gravimetric method for Class I mixtures, International Standard Organization, Geneva (Switzerland), 2015.
- [14] CCC Software: <https://www.inrim.it/en/services/software-and-databases/ccc-software>. Accessed: Apr. 28, 2025.