



ISTITUTO NAZIONALE DI RICERCA METROLOGICA Repository Istituzionale

Acoustic thermodynamic calibration of capsule-type standard resistance thermometers between 10 K and 25 K

Original

Acoustic thermodynamic calibration of capsule-type standard resistance thermometers between 10 K and 25 K / Gavioso, Roberto; Imbraguglio, Dario; MADONNA RIPA, DANIELE ANGELO; Steur, Peter. - (2023), pp. 190-190. (Intervento presentato al convegno Tenth International Temperature Symposium Anaheim, CA USA April 3-7, 2023).

Availability:

This version is available at: 11696/80180 since: 2024-03-01T17:37:40Z

Publisher:

Published

DOI:

Terms of use:

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

Publisher copyright

(Article begins on next page)

Acoustic thermodynamic calibration of capsule-type standard resistance thermometers between 10 K and 25 K

Roberto Gavioso¹, Dario Imbraguglio¹, Daniele Madonna Ripa¹, Peter Steur¹

¹Istituto Nazionale di Ricerca Metrologica (INRIM), Torino, Italy

Corresponding Author: r.gavioso@inrim.it

Gavioso ORCID: 0000-0002-1631-5133; Imbraguglio ORCID: 0000-0002-1289-772X

Madonna Ripa ORCID: 0000-0002-8760-8574; Steur ORCID: 0000-0001-5161-8554

In the context of the EMPIR research project “Realizing the Redefined Kelvin” (Real-K)¹ [1], we have implemented absolute acoustic gas thermometry [2] between 10 K and 25 K to evaluate the performance of this method for the direct thermodynamic calibration of capsule-type resistance thermometers on the thermodynamic temperature scale. Our implementation of acoustic thermometry is based on speed of sound measurements in He at a single pressure, chosen in the range between 65 kPa and 125 kPa, at each temperature calibration point, with non-ideality corrections relying on the accurate ab initio calculations of the thermophysical properties of He.

From the acoustic calibration of RhFe and Pt capsules, previously calibrated on ITS-90, we determine $(T-T_{90})$ differences between the thermodynamic temperature T and its approximation T_{90} by the International Temperature Scale of 1990 (ITS-90), finding them in remarkable agreement with the 2022 consensus estimate [3] of these differences within the small combined uncertainties.

We discuss the advantages of acoustic thermodynamic calibration compared to ITS-90 calibration both in terms of achievable uncertainty and practicality of use.

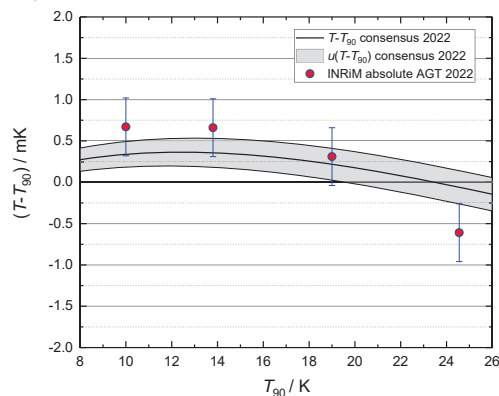


Fig. 1 Differences $(T-T_{90})$ determined using absolute acoustic gas thermometry between 10 K and 25 K.

References

- [1] G. Machin, M. Sadli, J. Pearce, J. Engert, R. M. Gavioso, “Towards realising the redefined kelvin”, Measurement 201, 111725 (2022) doi: [10.1016/j.measurement.2022.111725](https://doi.org/10.1016/j.measurement.2022.111725)
- [2] M. R. Moldover, R. M. Gavioso, J. B. Mehl, L. Pitre, M. de Podesta and J. T. Zhang "Acoustic Gas Thermometry", Metrologia, 51, R1-R19, (2014)
- [3] C. Gaiser, B. Fellmuth, R. M. Gavioso, M. Kalemci, V. Kytin, T. Nakano, A. Pokhodun, P. M. C. Rourke, R. Rusby, F. Sparasci, P. P. M. Steur, W. L. Tew, R. Underwood, R. White, I. Yang and J. Zhang “2022 Update for the Differences Between Thermodynamic Temperature and ITS-90 Below 335 K” J. Phys. Chem. Ref. Data 51 043105 (2022)

¹ The author is pleased to acknowledge support to produce this paper from the European metrology programme for innovation and research (EMPIR) project 18SIB02 “Realising the redefined kelvin” <https://real-k.aalto.fi/>