



## ISTITUTO NAZIONALE DI RICERCA METROLOGICA Repository Istituzionale

Automated DC voltage and DC resistance real-time multiple standard for artifact calibration of calibrators and multimeters

*Original*

Automated DC voltage and DC resistance real-time multiple standard for artifact calibration of calibrators and multimeters / Galliana, F.; Capra, P.; Cerri, R.; Francese, C.; Lanzillotti, M.; Roncaglione Tet, L.; Pennechi, F.; Pollarolo, A.. - In: JOURNAL OF INSTRUMENTATION. - ISSN 1748-0221. - 20:02(2025), pp. 1-9. [10.1088/1748-0221/20/02/p02002]

*Availability:*

This version is available at: 11696/84259 since: 2025-02-06T07:28:37Z

*Publisher:*

IOP

*Published*

DOI:10.1088/1748-0221/20/02/p02002

*Terms of use:*

This article is made available under terms and conditions as specified in the corresponding bibliographic description in the repository

*Publisher copyright*

Institute of Physics Publishing Ltd (IOP)

IOP Publishing Ltd is not responsible for any errors or omissions in this version of the manuscript or any version derived from it. The Version of Record is available online at DOI indicated above

(Article begins on next page)

PAPER • OPEN ACCESS

## Automated DC voltage and DC resistance real-time multiple standard for artifact calibration of calibrators and multimeters

To cite this article: F. Galliana *et al* 2025 *JINST* **20** P02002

View the [article online](#) for updates and enhancements.

You may also like

- [ANISOTROPIC LOCATIONS OF SATELLITE GALAXIES: CLUES TO THE ORIENTATIONS OF GALAXIES WITHIN THEIR DARK MATTER HALOS](#)  
Ingolfur Agustsson and Tereasa G. Brainerd
- [The Mid-Infrared Instrument for the James Webb Space Telescope, VI: The Medium Resolution Spectrometer](#)  
Martyn Wells, J.-W. Pel, Alistair Glasse et al.
- [Statistical equilibria of two-dimensional turbulent flows for generic initial vorticity fields on a sphere, calculated on the basis of the original Miller–Robert–Sommeria theory](#)  
K Ryono and K Ishioka



**UNITED THROUGH SCIENCE & TECHNOLOGY**

**ECS** The Electrochemical Society  
Advancing solid state & electrochemical science & technology

**248th  
ECS Meeting  
Chicago, IL  
October 12-16, 2025  
Hilton Chicago**

**Science +  
Technology +  
YOU!**

**SUBMIT  
ABSTRACTS by  
March 28, 2025**

**SUBMIT NOW**

The banner features a woman in a brown blazer smiling and gesturing. The background is blue with a network of white lines and nodes. The top and bottom of the banner are decorated with a repeating pattern of stylized circular icons.

# Automated DC voltage and DC resistance real-time multiple standard for artifact calibration of calibrators and multimeters

F. Galliana <sup>a,\*</sup> P. Capra <sup>a</sup> R. Cerri <sup>a</sup> C. Francese <sup>a</sup> M. Lanzillotti <sup>a</sup>  
L. Roncaglione Tet <sup>a</sup> F. Pennechi <sup>a</sup> and A. Pollarolo <sup>b</sup>

<sup>a</sup>Istituto Nazionale di Ricerca Metrologica (INRIM),  
Str. delle Cacce 91, 10135 Turin, Italy

<sup>b</sup>Measurements International Ltd. (MI),  
118 Commerce Drive Prescott, Ontario, Canada

E-mail: [f.galliana@inrim.it](mailto:f.galliana@inrim.it)

**ABSTRACT:** An automated temperature-controlled electrical DC voltage and DC resistance multiple reference standard (MRS) has been developed by Measurements International (MI) with the scientific support from the Istituto Nazionale di Ricerca Metrologica (INRIM). The MRS includes a 10 V, a 1  $\Omega$ , and a 10 k $\Omega$  standards selectable via a switch unit. This setup allows the artifact calibration of high-end calibrators and multimeters used in low-frequency electrical measurements. The two resistors are high-stability standards from MI, while the 10 V standard is based on a low-noise circuit developed by INRIM in collaboration with MI. A key innovation is the internal real-time clock calendar, which displays the calibration values of the MRS standards and their updated values internally calculated. This ensures reliable use of the MRS standards over extended periods between calibrations, effectively minimizing uncertainties due to their drift. The standards are housed in a thermal box, minimizing temperature variations. The MRS standards meet the uncertainty requirements defined by calibrators and multimeters manufacturers for artifact calibration and can also serve as laboratory references or travelling standards for interlaboratory comparisons (ILCs). MI is currently commercializing the MRS.

**KEYWORDS:** Detector alignment and calibration methods (lasers, sources, particle-beams); Analysis and statistical methods; Data analysis

\*Corresponding author.

---

## Contents

<b>1</b>	<b>Introduction</b>	<b>1</b>
<b>2</b>	<b>The MRS structure</b>	<b>2</b>
<b>3</b>	<b>The MRS standards</b>	<b>2</b>
<b>4</b>	<b>Calibration of the MRS standards</b>	<b>5</b>
<b>5</b>	<b>Using the MRS as a calibration standard</b>	<b>6</b>
<b>6</b>	<b>Algorithm to provide the real-time value of the standards</b>	<b>6</b>
<b>7</b>	<b>Measurement uncertainties</b>	<b>7</b>
<b>8</b>	<b>Conclusions</b>	<b>8</b>

---


## 1 Introduction

Standards and instruments require calibration with traceability to the International System of Units (SI) through national standards maintained by National Metrology Institutes (NMIs). Modern electrical digital instruments achieve traceability to the SI using a wide set of primary standards, such as DC voltage and resistors, DC and AC voltage dividers, AC/DC transfer standards, and current shunts, to cover wide measurement ranges. Alternatively, high-precision digital multimeters (DMMs), multifunction transfer standards (MTSs), or a limited set of primary standards can be employed [1]. In fact, high-end DMMs and multifunction calibrators (MFCs) can be calibrated with artifact calibration [2, 3], an in-house method requiring only three reference standards: 10 V, 1  $\Omega$ , and 10 k $\Omega$ . This procedure updates the internal references of DMMs and MFCs, which then automatically update other ranges and functions. However, since artifact calibration consists only of an adjustment of the references of the instruments, a full verification using a complete set of primary standards is periodically required to ensure their compliance with the manufacturer's specifications. At the Istituto Nazionale di Ricerca Metrologica (INRIM), portable temperature-controlled DC resistance setups for calibration of multifunction instruments were already realised [4, 5]. A first prototype of multiple DC Voltage and DC Resistance reference was developed at INRIM [6]. It was made up of two resistor networks and of a 10 V standard based on the LTZ 1000 circuit with the addition of 3D printed parts to maintain the stability of the integrated circuit at 48°C. After the development of this prototype, Measurements International (MI), with scientific and technical support from INRIM, has developed an automated, temperature-controlled, DC voltage and DC resistance real-time multiple reference standard (MRS) specifically designed for artifact calibration. The MRS includes a 10 V and a 1  $\Omega$  and a 10 k $\Omega$  resistors at single fruit. It employs a low-thermal-output scanner to select the artifact, minimizing electromotive forces (EMFs) and contact resistances during switching operations. The scanner also allows the automatic polarity reversal of the 10 V reference. The MRS provides key advantages to the user, including effective

thermal control and the ability to extrapolate real-time standard values. These features allow artifact calibrations to be performed at any time with uncertainties of the MRS standards comparable to their calibration ones. The MRS standards can also function as laboratory references in NMIs or travelling standards for interlaboratory comparisons (ILCs) [7], including high-level ones such as those in [8, 9].

## 2 The MRS structure

Figure 1 shows the block diagram of the MRS. The standards are housed in a temperature-controlled aluminium box, with the temperature monitored by an internal  $100\ \Omega$  Platinum Resistance Thermometer (PRT). The MRS has an internal battery and supports remote control via RS-232 or GPIB interfaces. According to the manufacturer, a recommended stabilisation period of 12 hours is required after powering on the MRS to ensure that its standards are ready for accurate measurements [10]. The selected standard is connected to the output via a LEMO-brand push-pull connector and a scanner, either for its calibration or as a reference for artifact calibration.

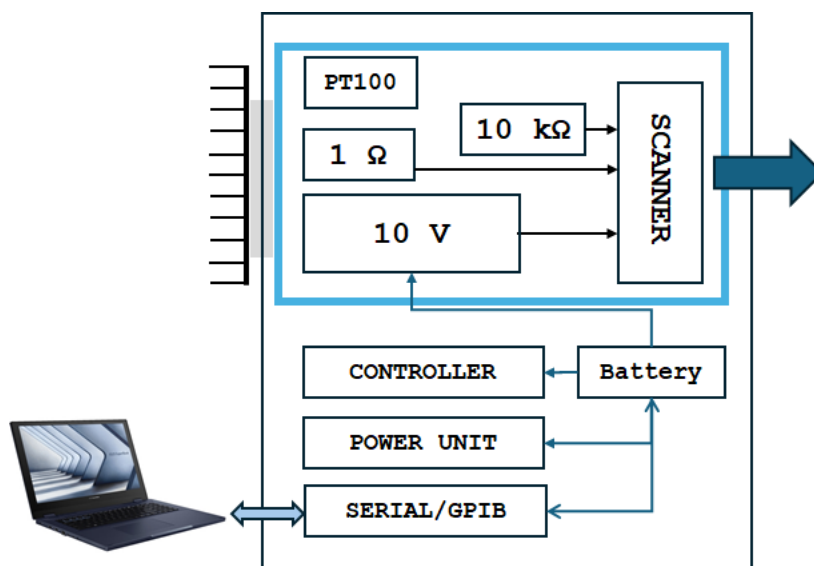

**Figure 1.** Simplified block diagram of the MRS. The three standards and the scanner are kept at constant temperature inside an electrostatic shield (blue box in the figure), and are separated from the electronic control and interfacing system and the power supply.

## 3 The MRS standards

Table 1 summarises the main specifications of the MRS standards, as provided in the manufacturer’s data sheet.

The resistors inside the MRS are manufactured by MI [10] and are based on well-established technologies. The  $1\ \Omega$  resistor is a bifilar non-inductive resistive element with low and negligible temperature and pressure coefficients. Its voltage terminals are welded using Evanohm [11] filler metal to minimise EMF. An annealing procedure is employed to reduce the temperature coefficient (TCR) of the resistor and for structural stabilisation the element is sealed in an oil-filled copper case. The  $10\ \text{k}\Omega$  resistor is instead of the metal foil type [12, 13]. The first prototype of the  $10\ \text{V}$  standard was

**Table 1.** Features of the MRS Standards declared by the manufacturer. \* For ambient temperatures in the range  $(23 \pm 5)$  C.

Standard	Temperature coefficient (TCR)*	Stability/Year	Dissipation
10 V	0.1 $\mu\text{V}/\text{V}/^\circ\text{C}$	1.5 $\mu\text{V}/\text{V}$	
1 $\Omega$	0.1 $\mu\Omega/\Omega/^\circ\text{C}$	0.5 $\mu\Omega/\Omega$	10 mW
10 k $\Omega$	0.1 $\mu\Omega/\Omega/^\circ\text{C}$	0.5 $\mu\Omega/\Omega$	10 mW

developed at INRIM. It utilised a temperature-stabilised Zener diode (Linear Technology LTZ1000) maintained at  $48^\circ\text{C}$  using an on-chip heater. Since the DC voltage reference is sensitive to thermal effects caused by contact points between the Zener pins and the printed circuit board tracks, the layout of the 10 V standard was specifically designed to minimise these effects. Within the MRS, the standards are anchored to a thermal mass maintained at  $35^\circ\text{C}$ . This stable temperature minimises thermal drift, thereby enhancing the long-term stability of the standards. At INRIM, the TCR of the 10 V standard was evaluated between  $18^\circ\text{C}$  and  $28^\circ\text{C}$  by placing a MRS in a thermo-regulated air bath with a stability better than  $\pm 0.01^\circ\text{C}$ . Table 2 shows the temperature dependence of the three standards. The TCR of the resistors was verified in the same controlled air bath, but prior to their integration into the MRS to verify if their TCR was suitable for the requirements of the MRS project.

**Table 2.** Temperature dependence of three reference standards. All the measurements were made inside the INRIM climatic chamber. The 10 V was measured inside the MRS case, while the resistors were measured outside the MRS case.

Temperature ( $^\circ\text{C}$ )	Values of relative deviation from nominal value ( $\times 10^{-6}$ )		
	10 V	1 $\Omega$	10 k $\Omega$
18	1.91		
19			
20	1.84		
21		9.8	-9.49
22	1.85		
23	2.04	10.1	-9.51
24	1.93		
25		10.2	-9.6
26	1.82		
27			
28	1.84		

The TCR of the 10 V standard has been conservatively estimated as approximately  $22 \text{ nV}/\text{V}/^\circ\text{C}$ . The TCRs of the 1  $\Omega$  and 10 k $\Omega$  resistors, assuming linear drift, have been estimated as about  $0.11 \mu\Omega/\Omega/^\circ\text{C}$  and  $0.16 \mu\Omega/\Omega/^\circ\text{C}$ , respectively. Placing the resistors in the MRS box further improves their TCR, thanks to the thermal control. Table 3 shows the mean measurements of the 10 V standard of an

MRS available at INRIM, maintained at 23°C inside a thermal chamber over a period of about three months. The drift was estimated to be approximately 2.8 nV/V/day (assuming a linear drift), a result reasonably consistent with the annual stability specified by the manufacturer. More accurate predictions of the 10 V standard's annual stability could be achieved using the methods outlined in [14–17]. However, this has been considered to be outside the scope of the work since users of the MRS can update the stability of their standards at each calibration. Table 4 shows the drift of the 10 V standard without thermal control in a laboratory thermally controlled at  $(23 \pm 0.5)^\circ\text{C}$ , measured immediately after powering on. This test was performed during the assembly phase of the 10 V prototype.


**Table 3.** Stability of the 10 V of an MRS measured at INRIM in the thermal chamber.

Date	Relative deviation from nominal value ( $\times 10^{-6}$ )
08/07	5.02
20/07	5.11
08/08	5.05
20/08	5.09
08/09	5.12
20/09	5.16

**Table 4.** INRIM measurements of a 10 V standard without thermal control after switching on.

Time	Measurements without thermal control from power on	Time	Measurements without thermal control from power on
(h)	Relative deviation from initial value ( $\times 10^{-6}$ )	(h)	Relative deviation from initial value ( $\times 10^{-6}$ )
1	0.03	8	0.16
2	0.09	9	0.15
3	0.11	10	0.18
4	0.14	11	0.20
5	0.17	12	0.18
6	0.15	13	0.17
7	0.18	14	0.16

The data in table 4 show that the drift of the 10 V standard without thermal control is significantly higher during the first seven hours after power-up, at approximately  $2.2 \times 10^{-8}$  per hour, and decreases to about  $1.4 \times 10^{-9}$  per hour between the 8th and 14th hour. Comparing these values with those in table 3, it can be concluded that the thermal control of the MRS, maintained at  $\pm 0.1^\circ\text{C}$ , combined with a stabilisation period of at least 12 hours prior to measurements, significantly improves the stability of this standard. This time period is also consistent with the stabilisation of DMMs/MFCs according to the manufacturers. Figures 2(a)–(d) show the long-term stability of the three standards of an MRS, beginning from its assembly. The measurements were performed at MI in a laboratory, thermally regulated at  $(23 \pm 0.5)^\circ\text{C}$ . The data show a significant drift during the first year and a half, probably due to the stabilisation process of the components. After this initial stabilisation period, the drift decreases and becomes more in line with the manufacturer's stability specifications.

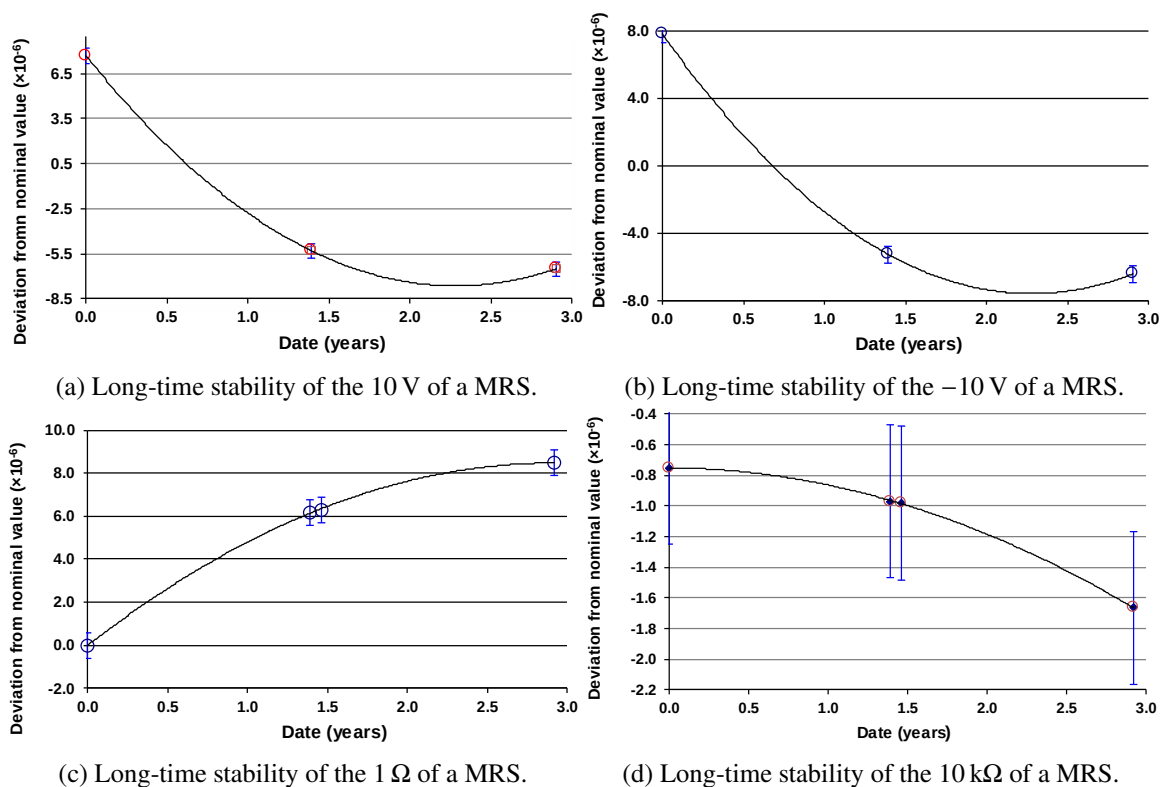

#### 4 Calibration of the MRS standards

The MRS standards must be calibrated with traceability to the SI through the DC voltage and DC resistance national standards according to the procedures and the quality system of the calibration laboratory. The 10 V standard can be calibrated either by comparison with a 10 V reference standard or through the Josephson effect [18] via a dedicated connection at room temperature, using a high-precision nanovoltmeter as a null detector. Similarly, the resistors can be calibrated with current comparator bridges by comparison with reference resistors traceable to the von Klitzing constant [19] or as a direct comparison to the quantum Hall effect using a cryogenic current comparator [20]. Table 5 reports the calibration results of the MRS standards obtained at INRIM during the period in which a MRS unit was available.


**Table 5.** Calibration results at INRIM of the standards of a MRS at  $23^\circ\text{C}$  in laboratory environment.

Nominal values	Calibration values	Measurement current mA	Relative expanded uncertainties ( $k = 2$ ) ( $\times 10^{-6}$ )
10 V	10.000051 V		0.5
$1 \Omega$	1.0000101 $\Omega$	100	0.5
10 k $\Omega$	9999.905 $\Omega$	0.1	0.5



## 5 Using the MRS as a calibration standard

Figure 3 shows a measurement setup for the artifact calibration of a MFC using the MRS standards. The connections and calibration steps are detailed in the user manuals of the instruments undergoing artifact calibration. For example, the Fluke 5720 MFC [21], after the artifact calibration and before saving the new constants, shows the changes of its internal references as  $\pm$  part per million (ppm). Table 6 provides a short report of an artifact calibration carried out at INRIM using the MRS standards.

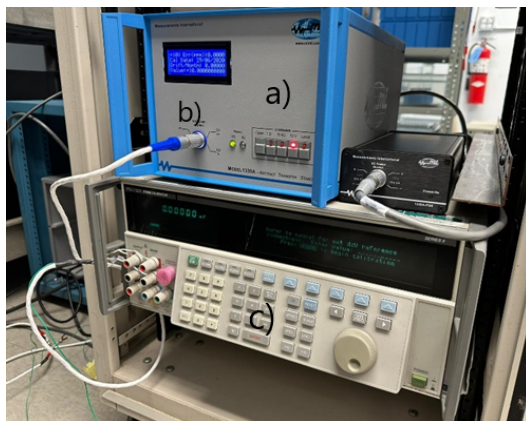

**Figure 3.** Photo of the measurement setup for the artifact calibration of a Fluke 5720 MFC (c) with the MRS (a). (b) is the LEMO connector. The connections to the LEMO connector are specifically designed to interface with the instruments in artifact calibration mode without requiring any modifications during the entire process. This design allows the calibration process to be fully automated, including zeroing.

**Table 6.** Short report of an artifact calibration of a Fluke 5720 MFC with the MRS standards at INRIM.

Standard	Reference values	J. Fluke 5720 reference changes (ppm)	
10 V MRS	10.000051 V	6.5 V	0.3
		13 V	-0.3
10 k $\Omega$ MRS	9.999905 k $\Omega$	10 k $\Omega$	0.1
1 $\Omega$ MRS	1.0000101 $\Omega$	1 $\Omega$	-2.9
		1.9 $\Omega$	-3.7

## 6 Algorithm to provide the real-time value of the standards

In general, when a laboratory calibrates DMMs and MFCs using artifact calibration, it is recommended to perform this process as soon as possible after the calibration of the 10 V, 1  $\Omega$ , and 10 k $\Omega$  reference standards to minimise their drift. Since the MRS's integrated algorithm provides real-time values for its standards, there is no need to perform the artifact calibration within a specific time frame after the calibration of the reference standards. The calibration values of the standards are stored in the MRS's control EPROM. By means of a real-time clock (RTC) and the algorithm, the MRS displays both the calibration values of the standards and their updated values. These updated values are calculated through an extrapolation process based on prior calibrations. The current version of the algorithm is simple: the user enters the calibration value of each standard, the calibration

dates, and the evaluated annual drifts. The algorithm then updates the values of the standards using a linear fit defined by equation (6.1).

$$X_d = X_{\text{cal}} + \left(d \frac{D}{365}\right) \quad (6.1)$$

where:

- $X_d$  is the value of a selected standard at the day  $d$ ;
- $X_{\text{cal}}$  is the last calibration value of the standard;
- $D$  is the estimated annual drift of the standard in relative parts;
- $d$  the number of days after the last calibration.

## 7 Measurement uncertainties

When an MRS standard is used in the time period between two its calibrations, its associated in-use uncertainties must be considered [22].<sup>1</sup> These uncertainties include contributions from calibration, drift, temperature variations, power, and transport effects. The implementation of the MRS algorithm significantly reduces the uncertainty component due to the drift. Table 7 shows the in-use uncertainty budgets for the three standards. The transport effect on the 10 V standard of an MRS, which is the most sensitive standard, was evaluated during an ILC among Canadian laboratories. It resulted less than  $4.0 \times 10^{-8}$ .

**Table 7.** In-use uncertainty budget according to [23] of the MRS standards (negl. indicates that the uncertainty contribution is negligible). \* According to [14], the pressure coefficient is  $0.025 \mu\Omega/\Omega$  in the 700–1200 hPa range, so, since the resistors are in a box and in a pressure-monitored laboratory, the contribution due to pressure can be considered negligible.

Standard	10 V	1 $\Omega$	10 k $\Omega$	Type and origin
Uncertainty component	Relative uncertainty ( $k = 1$ )			
Calibration	$2.5 \times 10^{-7}$	$2.5 \times 10^{-7}$	$2.5 \times 10^{-7}$	Normal B INRIM calibration
Drift	$2.4 \times 10^{-9}$	$7.9 \times 10^{-10}$	$7.9 \times 10^{-10}$	Rect. B MI spec. + algorithm
Temperature effect	$5.810^{-8}$	$5.8 \times 10^{-8}$	$5.8 \times 10^{-8}$	Rect. B MI spec.+ thermal reg.
Emf	$1.2 \times 10^{-8}$	$1.2 \times 10^{-7}$	negl.	Rect. B 20 $\mu\text{V}$ typical value
Power effect	—	$1.4 \times 10^{-7}$	$1.0 \times 10^{-7}$	Rect. B MI spec.
Pressure effect	negl.*	negl.	negl.	Rect. B [14]
Transport effect	$2.3 \times 10^{-8}$	$2.3 \times 10^{-8}$	$2.3 \times 10^{-8}$	Rect. B from ILC
$u_{\text{in-use}}(x_i) (k = 1)$	$2.5 \times 10^{-7}$	$3.1 \times 10^{-7}$	$2.5 \times 10^{-7}$	
$U_{\text{in-use}}(x_i) (k = 2)$	$0.5 \times 10^{-6}$	$0.6 \times 10^{-6}$	$0.5 \times 10^{-6}$	

<sup>1</sup>The concept of use uncertainty has been introduced since the calibration uncertainty of a standard could not be valid after some time after calibration. This is due to the standard drift and to the conditions in which the standard is used that could be different from those in which it was calibrated.

The uncertainty component due to the drift is negligible since the extrapolation function of the MRS values reduces this component to:

$$u_{\text{drift}} = \frac{\left(\frac{D}{365}\right)}{\sqrt{3}} \quad (7.1)$$

The values provided by the manufacturer (table 1) have been used for  $D$  in the uncertainty budget of table 7. Similar considerations apply to the uncertainty component related to the standards' temperature dependence, which is reduced by the thermo-regulation of the MRS. The in-use uncertainties of the MRS standards also apply when they are used as laboratory references during the interval between their calibrations.

## 8 Conclusions

The MRS is a versatile and efficient static and portable metrological reference unit. It represents an effective solution for the calibration (adjustment) of high-end digital multimeters and multifunction calibrators using artifact calibration. From a metrological point of view, the MRS specifications meet the uncertainty requirements of manufacturers of high-end MFCs and DMMs. Economically and logistically, the MRS offers significant advantages, making it a cost-effective and practical choice. The MRS can also be used as a travelling standard for ILCs for DC resistance and DC voltage measurements. Future efforts will focus on improving the data extrapolation algorithm to further increase the accuracy and reliability of the instrument as the number of calibrations increases.

## References

- [1] C. Cassiago, G. La Paglia and U. Pogliano, *Stability evaluation of high-precision multifunction instruments for traceability transfer*, *IEEE Trans. Instrum. Meas.* **49** (2000) 1206.
- [2] Fluke Corporation, *Calibration: Philosophy in Practice*, Second Edition (1994).
- [3] G. Rietveld et al., *Artifact calibration — An Evaluation of the Fluke 5700 A series II Calibrator*, Eindhoven, The Netherlands (1999), ISBN 90-9013322-4.
- [4] P.P. Capra and F. Galliana, *1  $\Omega$  and 10 k $\Omega$  high precision transportable setup to calibrate multifunction electrical instruments*, *Measurement* **82** (2016) 367 [[arXiv:1505.04398](https://arxiv.org/abs/1505.04398)].
- [5] P.P. Capra et al., *A temperature variable high accuracy 10 k $\Omega$  resistor*, *Metrol. Meas. Syst.* **16** (2009) 183.
- [6] P.P. Capra et al., *Portable DC Voltage and Resistance Reference with Switching Unit for Calibration of Electrical Precision Multifunction Instruments*, in the proceedings of the *2018 Conference on Precision Electromagnetic Measurements (CPEM 2018)*, Paris, France, July 8–13 (2018) [[DOI:10.1109/cpem.2018.8501092](https://doi.org/10.1109/cpem.2018.8501092)].
- [7] F. Galliana, *Measurement comparisons: A tool to guarantee the reliability of measurement systems and of high-tech industry*, *IEEE Instrum. Meas. Mag.* **22** (2019) 62.
- [8] F. Delahaye, D. Bournaud and T.J. Witt, *Report on the 1990 International Comparison of 1  $\Omega$  and 10 k $\Omega$  Resistance Standards at the BIPM*, *Metrologia* **29** (1992) 273.
- [9] D. Reymann et al., *Recent developments in BIPM voltage standard comparisons*, *IEEE Trans. Instrum. Meas.* **50** (2001) 206.
- [10] Measurement International, *Artifact Transfer Standard Model 1330A operator manual, rev. 5*, 2023.

- [11] B.J. Pritchard and R.C. Grime, *Fabrication of reference standard 1 ohm resistors from Evanohm S alloy*, in the proceedings of the *Conference on Precision Electromagnetic Measurements*, Ottawa, ON, Canada, June 11–14 (1990) [DOI:10.1109/cpem.1990.110027].
- [12] Y. Sakamoto et al., *Novel 100-Ω Metal Foil Resistor*, *IEEE Trans. Instrum. Meas.* **60** (2011) 2544.
- [13] A. Domae et al., *Characterization of 100-Ω Metal Foil Standard Resistors*, *IEEE Trans. Instrum. Meas.* **62** (2013) 1776.
- [14] A. Bartašiunas, R. Miškinis, D. Smirnov and E. Urba, *Stability and predictability of Zener reference voltage standards: long-term experience by the Lithuanian National Metrology Institute*, *Metrolog. Meas. Syst.* **31** (2024) 434.
- [15] D. Ilić, A. Šala and I. Leniček, *Prediction of the output Voltage of dc voltage standards*, in the proceedings of the *XIX IMEKO World Congress on Fundamental and Applied Metrology*, Lisbon, Portugal, September 6–11 (2009), pp. 601–606.
- [16] S.-N. Park, H.-S. Shim, H. Cho and M.-S. Kim, *Long-term drift analysis of Zener voltage standards and proposal of an initial calibration interval using calibration records accumulated for 15 years*, *Metrologia* **57** (2020) 065007.
- [17] O. Power and J.E. Walsh, *Investigation of the Long- and Medium-Term Drift of Zener Diode-Based Voltage Standards*, *IEEE Trans. Instrum. Meas.* **54** (2005) 330.
- [18] R. Pöpel, *The Josephson Effect and Voltage Standards*, *Metrologia* **29** (1992) 153.
- [19] K. von Klitzing, G. Dorda and M. Pepper, *New method for high accuracy determination of the fine structure constant based on quantized Hall resistance*, *Phys. Rev. Lett.* **45** (1980) 494.
- [20] J.M. Williams, T.J.B.M. Janssen, G. Rietveld and E. Houtzager, *An automated cryogenic current comparator resistance ratio bridge for routine resistance measurements*, *Metrologia* **47** (2010) 167.
- [21] Fluke, *5700A/5720A Series II Multi-Function Calibrator*, 2002.
- [22] W. Bich and F. Pennecchi, *On the in-use uncertainty of an instrument*, in the proceedings of the *Advanced Mathematical and Computational Tools in Metrology VI*, Torino, Italy, September 1 (2003), pp. 159–169 [DOI:10.1142/9789812702647\_0013].
- [23] *JCGM 100:2008. Evaluation of measurement data — Guide to the expression of uncertainty in measurement*, first edition, 2008